


**RECOMMENDED
DEVICE SETUP
IN LEO 2.0
FOR GAS
MEASUREMENT**



PRECAUTIONS:

- Please be cautious with your cultured embryos, considering that during the measurement procedure the composition of the gas in the chamber may be affected.
- Read the manuals for the incubator and LEO 2.0 for usage and safety details.

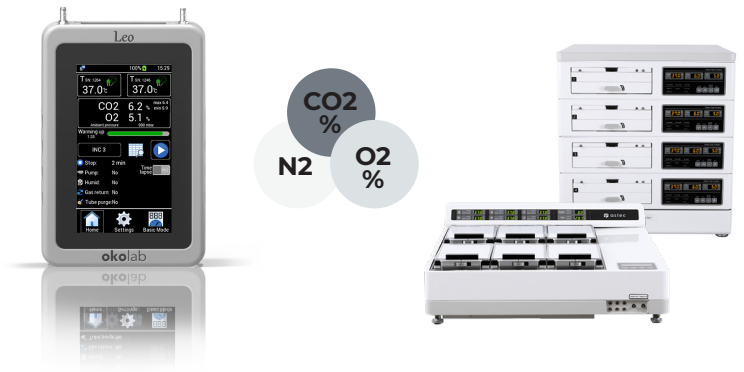

Evaluate the need for chamber cleaning and disinfection after working on the incubator.



As good practice, it is recommended to have LEO 2.0 charged before use, and not to charge it during use.



Always read the manual of the devices.




If LEO 2.0 shows a message that it's warming up, it is advised to complete the warm up period before using.

STEP 1


Connect TUBE-A to LEO 2.0's **IN** port and to the **ASTEC** gas Sample Out port.

Connect the OUTPUT-TUBE to LEO 2.0's **OUT** port and to the **gas Sample IN** port of **ASTEC** to return the gas.

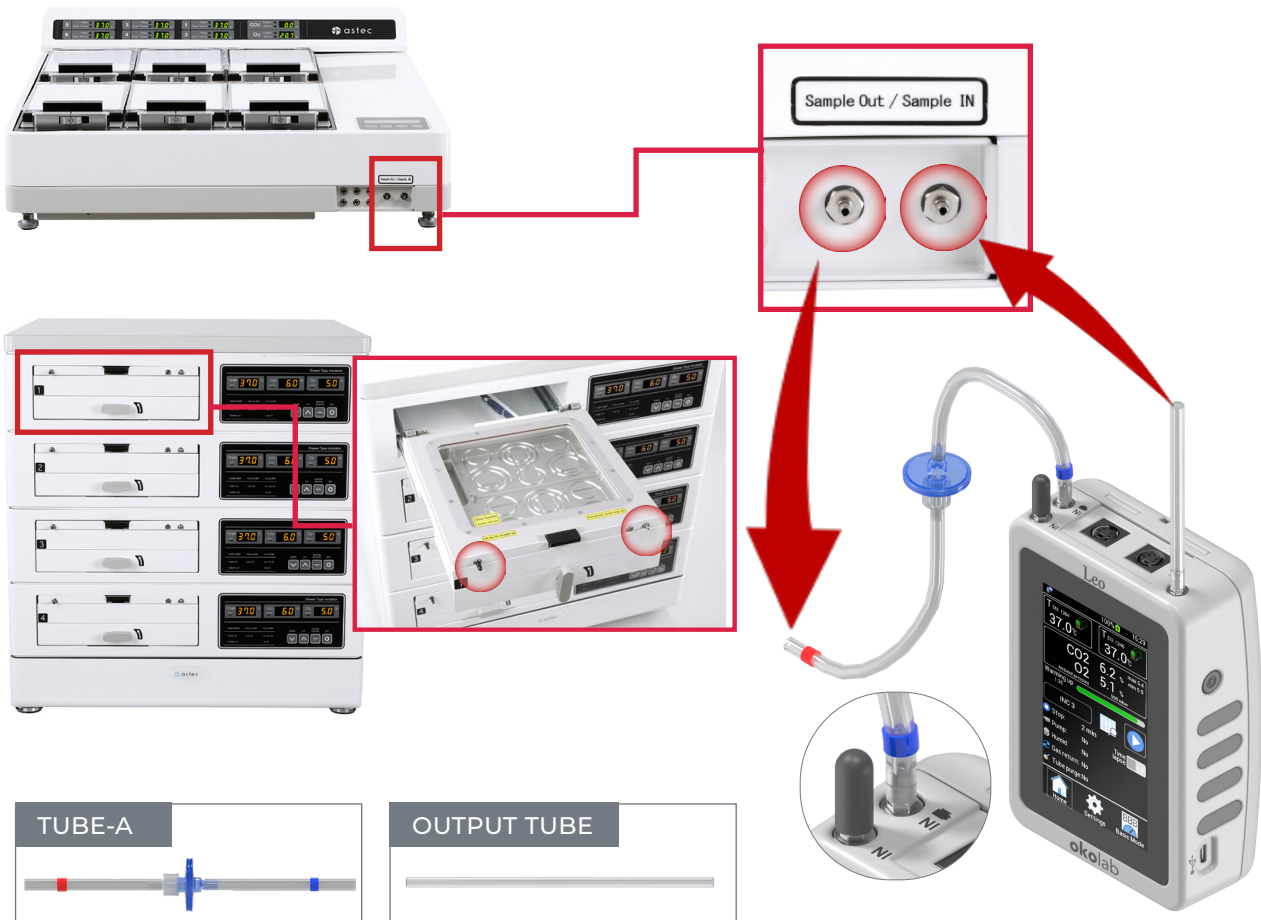


TUBE-A


OUTPUT TUBE

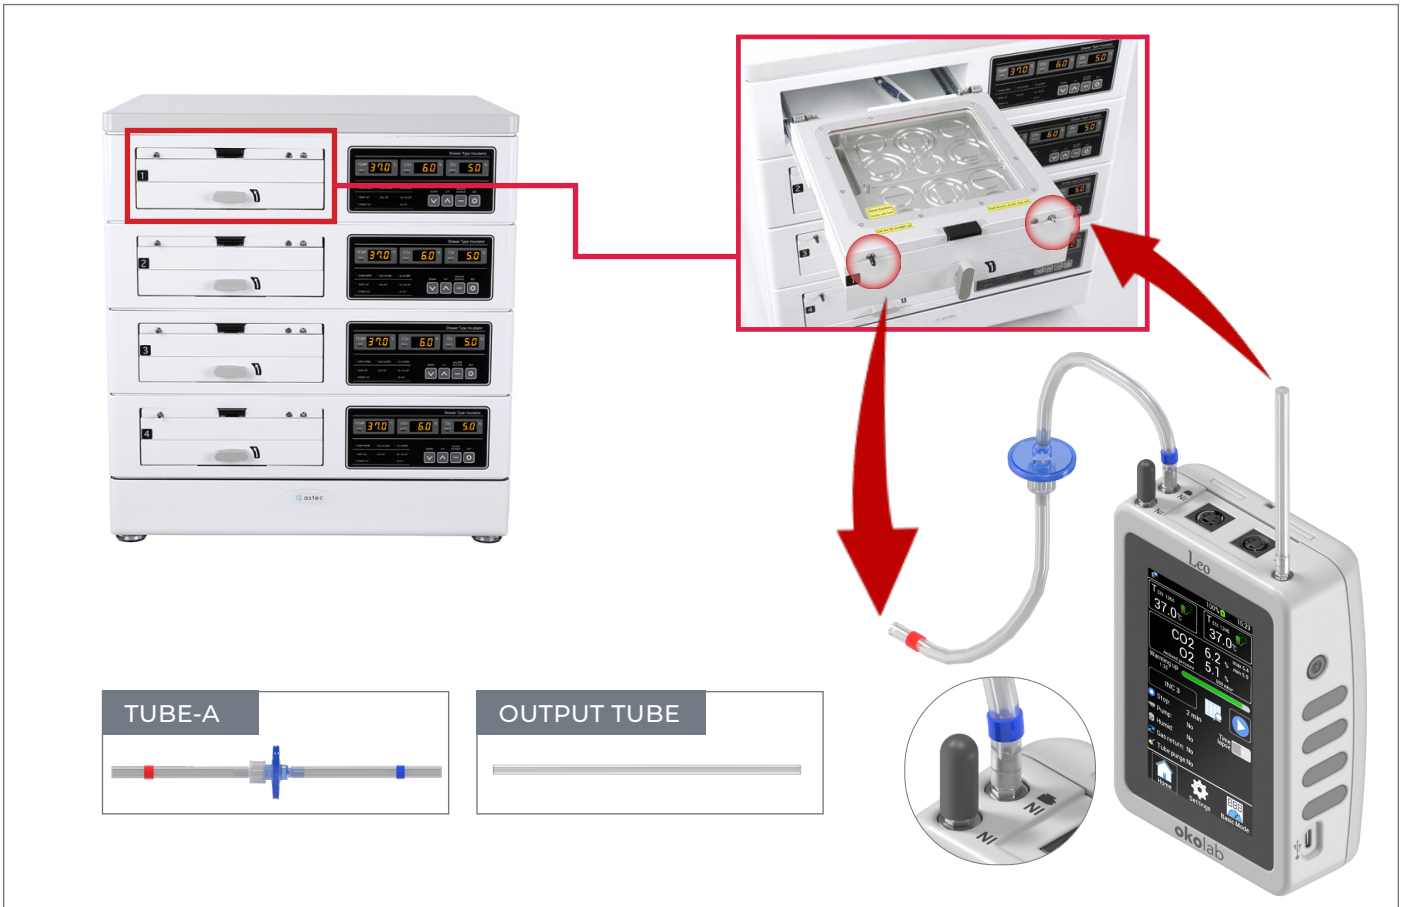

STEP 2 Select Device.

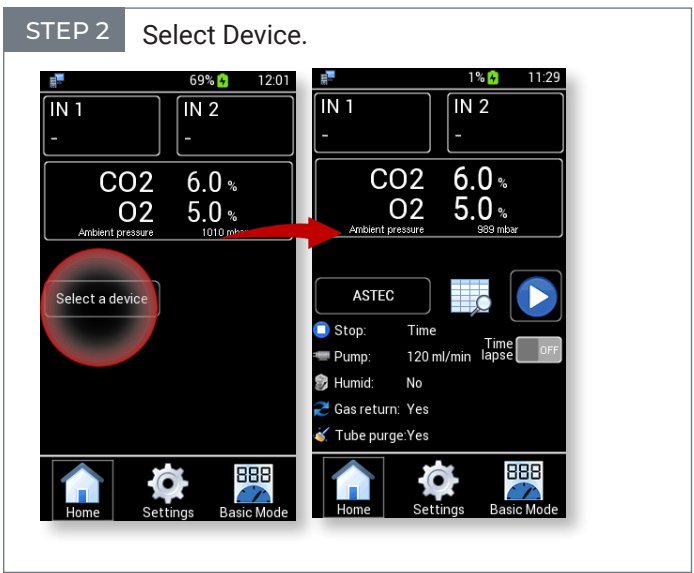

STEP 3 Give at least 10 minutes for **ASTEC** to stabilize the gas concentration in the chambers. Do not open the lids.

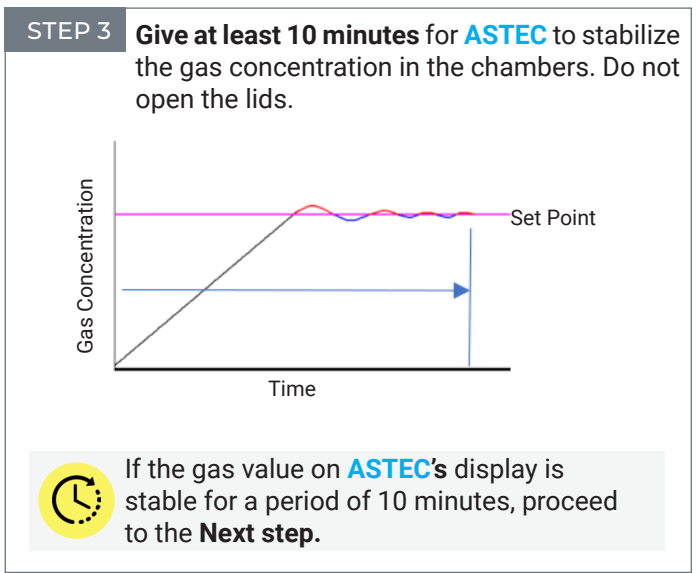

If the gas value on **ASTEC**'s display is stable for a period of 10 minutes, proceed to the **Next** step.

STEP 4 Start a **LEO 2.0** gas measurement.

